


- NOTES**
- REFER TO APPROPRIATE DATA SHEET FOR BACKBOX REQUIREMENTS. ALL BOXES TO BE U.L. LISTED.
 - MINIMUM WIRE SIZE IS AWG FOR ALL COMMON CONDUCTORS AND 22 AWG FOR ALL OTHERS INCLUDING AUDIO CABLES.
 - USE GREEN CONDUCTOR FOR GROUND ONLY.
 - MAXIMUM CONTROL OUTPUT 24 VDC 3 AMPS.
 - ALL BUILDING WIRES MUST BE FREE OF GROUNDS PRIOR TO CONNECTING TO TS 4.
 - DO NOT CONNECT TO EARTH GROUND AT ANY POINT.

WIRE COLOR CODE

RD	RED
BK	BLACK
BR	BROWN
BL	BLUE
GR	GREEN
OR	ORANGE
YL	YELLOW
WH	WHITE
SL	SLATE

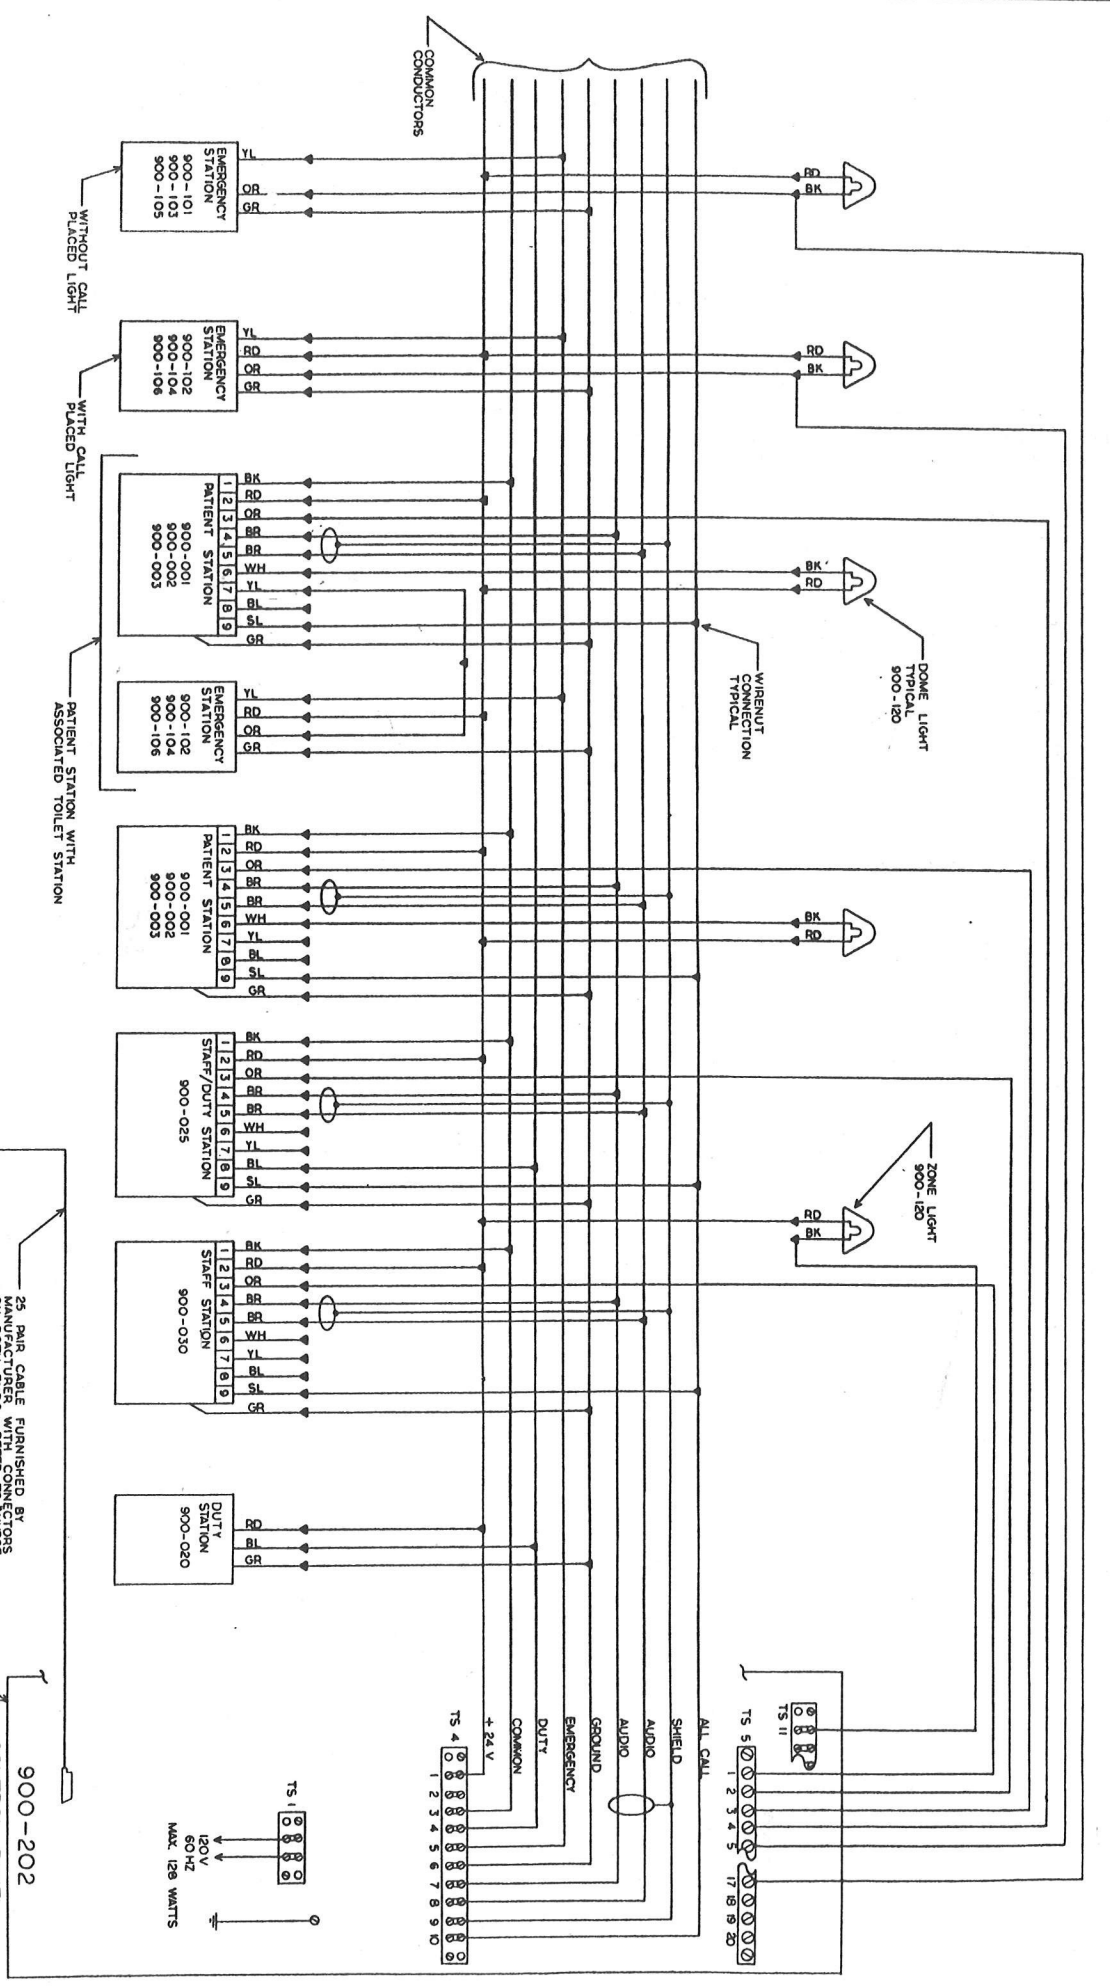

25 PAIR CABLE FURNISHED BY MANUFACTURER. WIRE GAUGE ON BOTH ENDS. REFER TO NURSE STATION MASTERS' DATA SHEET FOR NECESSARY CABLE AND CONDUIT REQUIREMENTS.

CONTROL CABINET FURNISHED BY THE 100-820 24" H X 18" W X 4.5" D

ENGINEERED ELECTRONICS INC.
 P. O. BOX 60 DOUGLASVILLE, GA. 30134

PROJECT FIELD WIRE CONNECTIONS
 AUDIO/VISUAL NURSE CALL SYSTEM

DATE 5-3-63
 SCALE NONE
 DWG BY
 SHEET 1 OF 1

DRAWING 383-002